


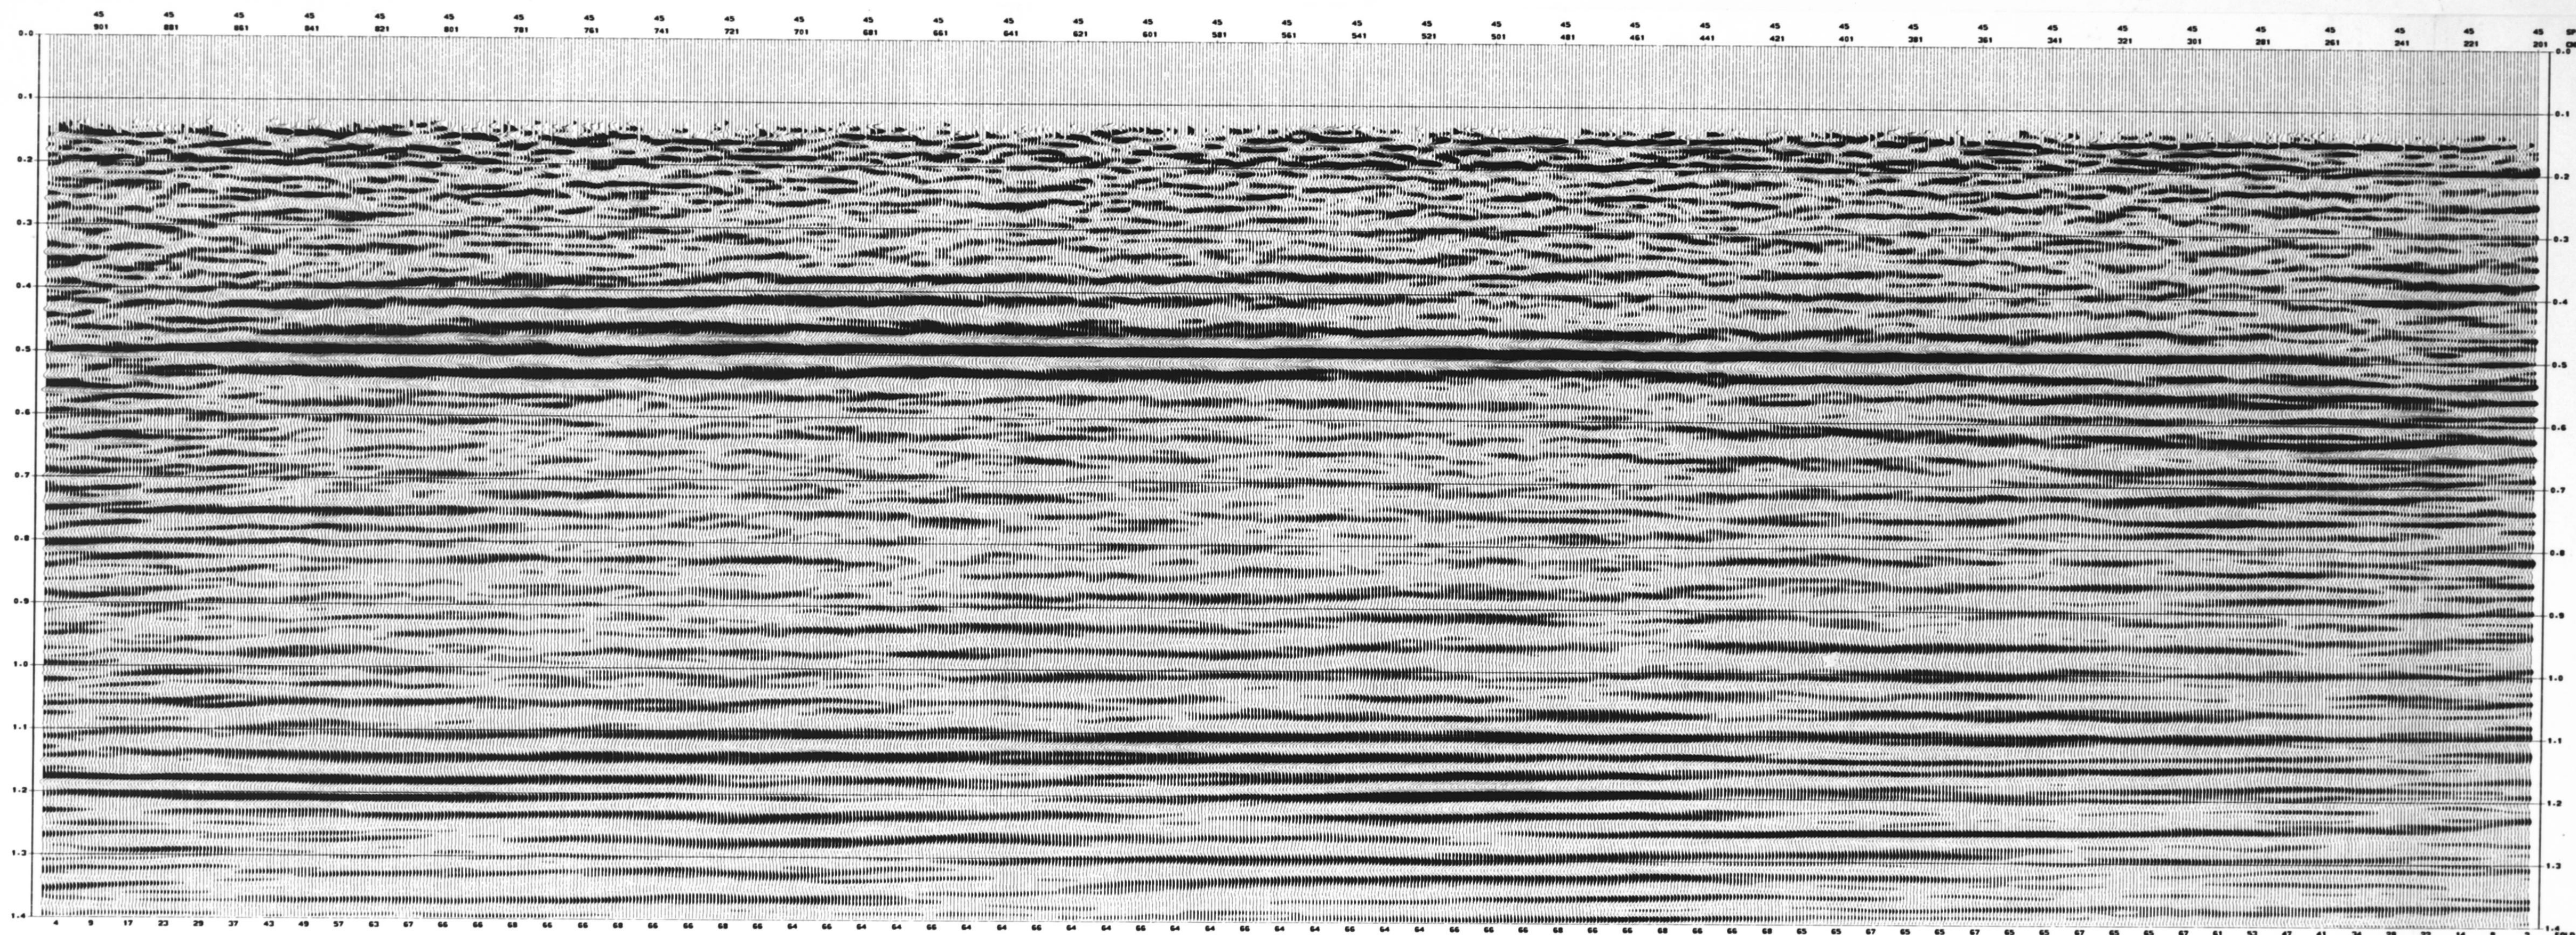

9229-J1-6E

Line Marker
Sample Interval: 2000
Number of Samples: 791
Sample Rate: 1
CP Field